

US1-Symphony Bone Level


**Product Catalog | 2026** 









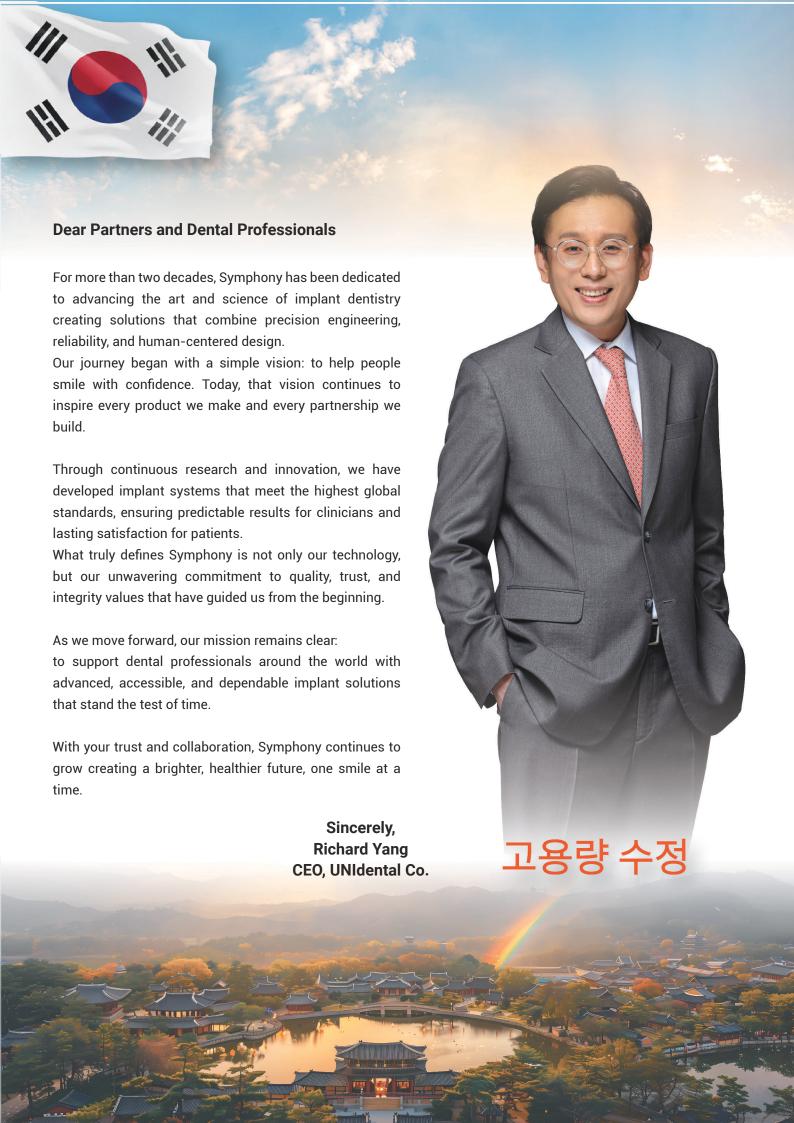


## SYMPHONY IMPLANT

Symphony implant a product of UNIdental.Co.,Ltd company. UNIdental

Develops and produces implant system more than 20 years.

UNIdental.Co.,Ltd Develops and produces a product with the motto of providing the best products and services by R&D professionals who have worked for research,

development, and production of dental products and Implant-related areas Sincs 2002.











#### SYMPHONY NETWORK

Driven by exceptional feedback from dentists around the world, Symphony Implant continues to strengthen its global footprint. With sales and representation in nearly 20 countries, the brand is now strategically expanding its presence in the United States - bringing Korean innovation and precision to dental practices across the globe.





#### **EUROPE**



Hungary



Georgia



Albania





Norway



Turkey

#### ASIA



Korea



China



Vietnam



Thailand

#### **MIDDLE EAST**



Saudi Arabic



Iraq



Pakistan

#### **AMERICA**



**United States** 



Mexico



#### CIS



Russia



Uzbekistan



# **SURFACE INNOVATION & GLOBAL PATENTS**




At Symphony Implant, innovation begins at the microscopic level.

Through continuous research and technological advancement, Symphony has developed a unique surface treatment and cleaning technology designed to optimize osseointegration and long-term implant stability.

This proprietary technology effectively removes residual contaminants from the implant surface while enhancing surface energy and purity — resulting in faster bone healing and greater clinical success.


Our innovation has been officially patented in the United States, Japan, and South Korea, reflecting the originality and scientific excellence of our R&D process.


With this patented technology, Symphony ensures every implant is not only clean — but biologically ready to perform.

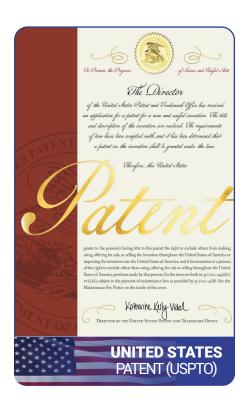















#### **UNI**dental **R&D**

Due to the high variety of implant products and the speed of development of this industry in the world, **UNI**dental's research and development department is one of the most important departments of **UNI**dental company, which is under the supervision of specialists in surface engineering, materials, biology, as well as prominent dental specialists, including a group of oral and maxillofacial surgeon as well as periodontology specialists and prosthetics from Prominent universities in the world are working hard to improve the products as well as to develop and expand the dental implants of **UNI**dental company.




One of the most important needs in medical and biological products is to take advantage of the expertise and the needs of dental experts to create products according to the needs of the dental community according to the needs of this group. **UNI**dental research and development specialists are regularly updating this knowledge based on the standard criteria of this field.


## **SYMPHONY Packaging**

In the packaging of SYMPHONY products, all diameters are separated based on colors.

All the specifications are listed on the packaging, which can also be seen in the picture below.



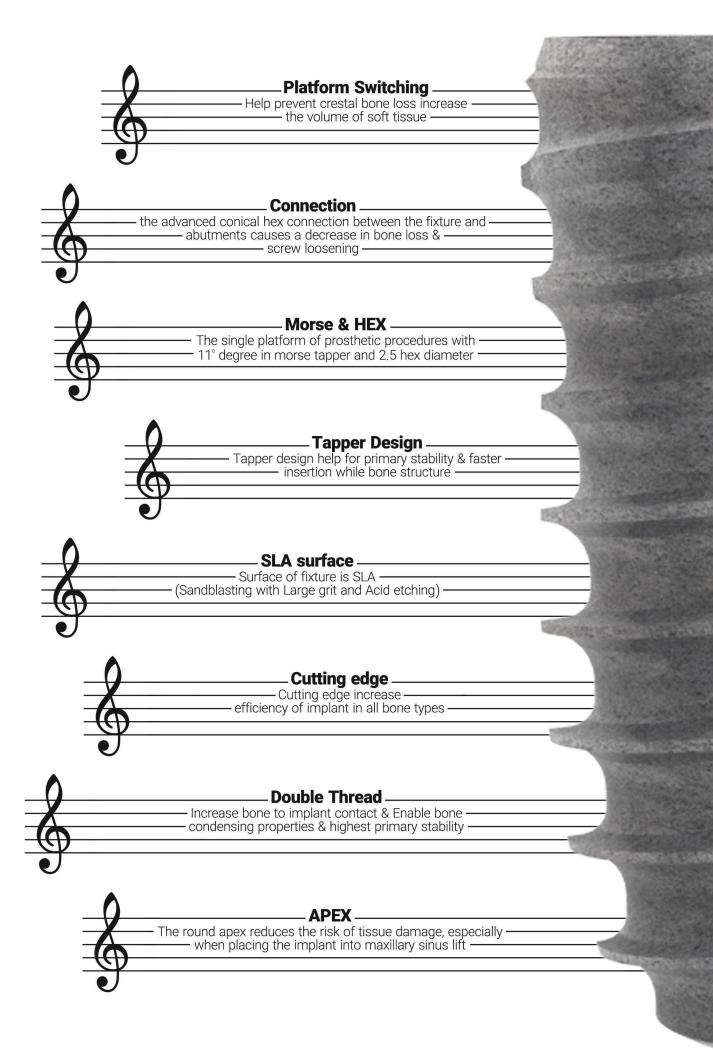

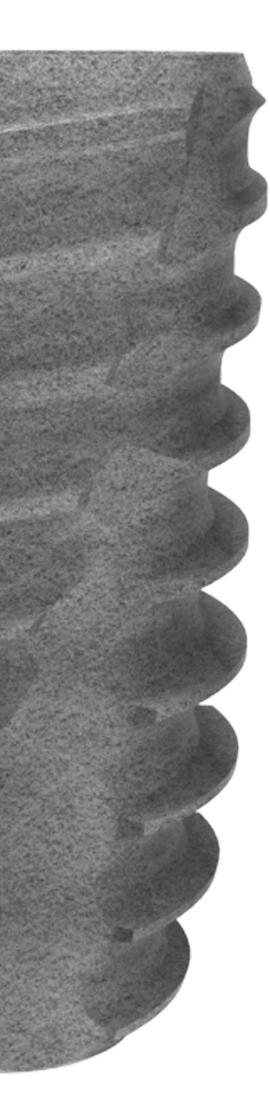

## SYMPHONY S.L.A surface feature

The surface treatment of **SYMPHONY** implants is S.L.A (Sandblasting with Large grit and Acid etching). This surface treatment technology causes:


- Higher BIC (Bone to Implant Contact)
- Faster and Stronger Osseointegration


Optimal surface through Acid etching Ideal surface RA 2.0~3.0µmm

- More 45% surface area than RBM
- More than 20% enhanced activation of Osteoblast & Bone formation than RBM


Superior Osseointegration In-vivo experiment [mini-pig]

- Enhanced 45% of early fixation against RBM
- Enhanced 20% of new bone formation against RBM [BIC, 4wks]
- Macropore and Micropore of Titanium Oxide layer Mimicking the etched enamel rod of tooth
- Uniform distribution of roughness on whole length of fixture
- Hydrophilic wettability activated with rinsing solution





SEM image of SYMPHONY fixture



roughness analysis of SYMPHONY fixture

## Content

#### Symphony 1 Implant System

(Bone Level)



Fixture / Cover Screw	02	Symphony 1 Surgical kit	26
Healing Abutment	04	Symphony Prosthetic Kit	29
Prosthetic Procedure I & II	06	Symphony All Surgical Kit	30
Dual Abutment (Hex & Non-Hex)	08		
Angled Abutment (Hex & None-Hex)	12		
Temporary Abutment	14		
CCM Abutment	14	Cymarkany	
Lab Analog	15	Symphony Protocol	
Ti-base Abutment (for Cerec)	15	Frotocor	
Impression Coping Components	16		
Multi Straight Abutment	18	Symphony 1 Surgical Protocol	32
Multi Angled Abutment	18		
Multi Temporary Abutment	19		
Multi CCM Abutment	19		
Multi Impression Coping	20		
Multi Lab Analog	20		
Ball Abutment	21		
Kerator Abutment	22		



## **Fixture**

#### Optimized Design for ANY SURGERY

- Simple surgical protocol helps reduce chair time
- Stabilized in use to Extraction Socket
- Enables Early Loading in upper posterior
- Titanium Grade 4

#### **Dual & Deep Thread**

- Enhancing initial stability from deeply designed Thread
- Dual thread enables Fast insertion

#### **Tapered Design**

- Similar design of natural tooth
- · Proper load distribution harmonized with anatomy

#### Surgery Speed & Torque

For drilling use: 800-1200 Rpm / 30-40 N
For fixture insertion: 30 Rpm / 30-40 N



body diameter

Coding Sample: US1-4008



All Fixture's size have 2.5 Hex Diameter

Platform Ø 3.6

Body Ø 3.8

Code	US1-3607B	US1-3607	US1-3608	US1-3610	US1-3612	US1-3614
L	7B	7	8	10	12	14

Platform Ø 4.0

Body Ø 3.8

Code	US1-4007B	US1-4007	US1-4008	US1-4010	US1-4012	US1-4014
L	7B	7	8	10	12	14

#### Platform Ø 4.5 Code US1-4507B US1-4507 US1-4508 US1-4510 US1-4512 US1-4514 L 7В 8 10 12 14 Body Ø 4.3 Platform Ø 5.0 US1-5007B US1-5007 US1-5008 US1-5010 US1-5012 US1-5014 Code L 7В 7 8 Body Ø 4.8 10 12 14 Platform Ø 6.0 US1-6007B UST-6007 US1-6008 US1-6010 US1-6012 Code Body Ø 4.8 L 7В 7 8 10 12 US1-7007B Platform Ø 7.0 US1-7007 US1-7008 US1-7010 US1-7012 Code L 7В 8 10 12 Body Ø 5.8

## **Cover Screw**

- Using a 1.28 Hex driver
- Recommended torque for fastening: ≤ 5Ncm
- Packaging and ordering: It is embedded in the upper part of the Fixture and for ordering use US1CS code with the desired size
- Scale of pic is 1:1.5mm
- Titanium Grade 5

#### Code

US1CS-36



## **Healing Abutment**

- Using a 1.28 Hex driver
- Recommended torque for fastening : ≤ 5Ncm
- Packaging and ordering: There is one piece in the package and to order use US1HA code with the desired size
- Scale of pic is 1:1.5mm



Coding Sample: US1HA-554070

Diameter Ø 4.0	Code	G/H	н	Pic.
	US1HA-402020	2	2.0	G/H <b>H</b> 7.0
	US1HA-402035	2	3.5	<b>G/H</b> 4.0 High
	US1HA-403050	3	5.0	
	US1HA-404070	4	7.0	US1HA-404070
Diameter Ø 4.5	Code	G/H	н	Pic.
	US1HA-452020	2	2.0	<b>G/H H</b> 7.0
	US1HA-452035	2	3.5	<b>G/H</b> 4.0 High
	US1HA-453050	3	5.0	
	US1HA-454070	4	7.0	US1HA-454070
Diameter Ø 5.5	Code	G/H	н	Pic.
	US1HA-552020	2	2.0	<b>H</b> 7.0
	US1HA-552035	2	3.5	<b>G/H</b> 4.0
	US1HA-553050	3	5.0	
	US1HA-554070	4	7.0	US1HA-554070

#### Diameter Ø 6.5

Code	G/H	Н
US1HA-652020	2	2.0
US1HA-652035	2	3.5
US1HA-653050	3	5.0
US1HA-654070	4	7.0



Pic.

#### Diameter Ø 7.5

Code	G/H	Н
US1HA-752035	2	3.5
US1HA-753050	3	5.0



Pic.

#### Diameter Ø 8.5

Code	G/H	Н
US1HA-852035	2	3.5
US1HA-853050	3	5.0



#### Diameter Ø 9.5

Code	G/H	н	Pic.
US1HA-952035	2	3.5	<b>H</b> 5.0
US1HA-953050	3	5.0	<b>G/H</b> 3.0
			B00000
			US1HA-953050

## **Prosthetic Procedure I**



## **Prosthetic Procedure II**

CCM Multi Multi Multi Temporary Abutment **Abutment** Straght **Angeld Abutment Abutment** Hex/Non-Hex Hex/Non-Hex USML-48 US1MT-4815H US1DA-4725H US1MA-481710H P 19 P 14 P 18 P 18 Multi Analog US1MC-4815H P 19 Multi **Impression** Coping USMI-P4811 P 20 Cover Healing **Screw Abutment** US1CS-36 US1HA-454070 P 02 P 04 **Fixture** Level

> US1-4008 P 02-03

## **Dual Abutment**

## Нех

Use for making general cemented type prosthetic

Gold coated for aesthetic effect

11° tapered connection

Using a 1.28 Hex driver

Recommended tourqe for fastening: ≤ 30Ncm

Packaging and order: There are two pieces in the package (abutment with screw).

and for order use US1DA code with the desired size

Available in both hex and non-hex

Scale of pic is 1:1.5mm

Titanium Grade 5



Coding Sample: US1DA-5725H

Diameter Ø 4.5	Code	G/H	н	Pic.
	US1DA-4510H	1.0	5.5	
	US1DA-4515H	1.5	5.5	<b>H</b> 5.5
	US1DA-4525H	2.5	5.5	<b>G/H</b> 2.5
	US1DA-4535H	3.5	5.5	US1DA-4525H
	US1DA-4545H	4.5	5.5	Hex
	US1DA-4555H	5.5	5.5	
	US1DA-4715H	1.5	7.0	
	US1DA-4725H	2.5	7.0	<b>H</b> 7.0
	US1DA-4735H	3.5	7.0	<b>G/H</b> 2.5
	US1DA-4745H	4.5	7.0	US1DA-4725H
	US1DA-4755H	5.5	7.0	Hex

Diameter Ø 5.5	Code	G/H	н	Pic.
	US1DA-5415H	1.5	4.0	<b>H</b> 4.0
	US1DA-5425H	2.5	4.0	<b>G/H</b> 2.5
	US1DA-5435H	3.5	4.0	- 1
	US1DA-5445H	4.5	4.0	<b>US1DA-5425H</b> Hex
	US1DA-5455H	5.5	4.0	
	US1DA-5515H	1.5	5.5	<b>H</b> 5.5
	US1DA-5525H	2.5	5.5	G/H
	US1DA-5535H	3.5	5.5	2.5
	US1DA-5545H	4.5	5.5	<b>US1DA-5525H</b> Hex
	US1DA-5555H	5.5	5.5	TIEX
	US1DA-5715H	1.5	7.0	<b>H</b> 7.0
	US1DA-5725H	2.5	7.0	1.7.5
	US1DA-5735H	3.5	7.0	<b>G/H</b> 2.5
	US1DA-5745H	4.5	7.0	1
	US1DA-5755H	5.5	7.0	<b>US1DA-5725H</b> Hex

Diameter Ø 6.5	Code	G/H	Н	Pic.
	US1DA-6415H	1.5	4.0	<b>H</b> 4.0
	US1DA-6425H	2.5	4.0	<b>G/H</b> 2.5
	US1DA-6435H	3.5	4.0	US1DA-6425H
	US1DA-6445H	4.5	4.0	Hex
	US1DA-6455H	5.5	4.0	
	US1DA-6515H	1.5	5.5	
	US1DA-6525H	2.5	5.5	<b>H</b> 5.5
	US1DA-6535H	3.5	5.5	<b>G/H</b> 2.5
	US1DA-6545H	4.5	5.5	
	US1DA-6555H	5.5	5.5	<b>US1DA-6525H</b> Hex

## **Dual Abutment**

## Non-Hex

Use for making general cemented type prosthetic Gold coated for aesthetic effect 11° tapered connection

Using a 1.28 Hex driver


Recommended tourge for fastening: ≤ 30Ncm

Packaging and order: There are two pieces in the package (abutment with screw).

and for order use US1DA code with the desired size

Available in both hex and non-hex

Scale of pic is 1:1.5mm



**Coding Sample: US1DA-4525N** 

Diameter Ø 4.5	Code	G/H	н	Pic.
	US1DA-4510N	1.0	5.5	
	US1DA-4515N	1.5	5.5	<b>H</b> 5.5
	US1DA-4525N	2.5	5.5	<b>G/H</b> 2.5
	US1DA-4535N	3.5	5.5	US1DA-4525N
	US1DA-4545N	4.5	5.5	Non-Hex
	US1DA-4555N	5.5	5.5	
	US1DA-4715N	1.5	7.0	
	US1DA-4725N	2.5	7.0	<b>H</b> 7.0
	US1DA-4735N	3.5	7.0	<b>G/H</b> 2.5
	US1DA-4745N	4.5	7.0	1
	US1DA-4755N	5.5	7.0	<b>US1DA-4725N</b> Non-Hex

Diameter Ø 5.5	Code	G/H	н	Pic.
	US1DA-5415N	1.5	4.0	<b>H</b> 4.0
	US1DA-5425N	2.5	4.0	<b>G/H</b> 2.5
	US1DA-5435N	3.5	4.0	
	US1DA-5445N	4.5	4.0	<b>US1DA-5425N</b> Non-Hex
	US1DA-5455N	5.5	4.0	
	US1DA-5515N	1.5	5.5	
	US1DA-5525N	2.5	5.5	<b>H</b> 5.5
	US1DA-5535N	3.5	5.5	<b>G/H</b> 2.5
	US1DA-5545N	4.5	5.5	US1DA-5525N
	US1DA-5555N	5.5	5.5	Non-Hex
	US1DA-5715N	1.5	7.0	
	US1DA-5725N	2.5	7.0	<b>H</b> 7.0
	US1DA-5735N	3.5	7.0	G/H
	US1DA-5745N	4.5	7.0	2.5
	US1DA-5755N	5.5	7.0	<b>US1DA-5725N</b> Non-Hex

Diameter Ø 6.5	Code	G/H	н	Pic.
	US1DA-6410N	1.0	4.0	<b>H</b> 4.0
	US1DA-6415N	1.5	4.0	<b>G/H</b> 2.5
	US1DA-6425N	2.5	4.0	2.0
	US1DA-6435N	3.5	4.0	<b>US1DA-6425N</b> Non-Hex
	US1DA-6445N	4.5	4.0	
	US1DA-6455N	5.5	4.0	
	US1DA-6510N	1.0	5.5	
	US1DA-6515N	1.5	5.5	<b>H</b> 5.5
	US1DA-6525N	2.5	5.5	<b>G/H</b> 2.5
	US1DA-6535N	3.5	5.5	US1DA-6525N
	US1DA-6545N	4.5	5.5	Non-Hex
	US1DA-6555N	5.5	5.5	

## **Angled Abutment**

## Hex & Non-Hex

Use for the path adjustment of prosthetic

Gold coated for aesthetic effect

11° tapered connection

2 Kinds of angulations, 15° and 25°

Using a 1.28 Hex driver


Recommended tourqe for fastening: ≤ 30Ncm

Packaging and order: There are two pieces in the package (abutment with screw).

and for order use US1AA code with the desired size

Scale of pic is 1:1.5mm

Titanium Grade 5



Coding Sample: U1AA-551525H

Diameter Ø	4.
Angled 15°	

Code	G/H	Connection Type
US1AA-451515H	1.5	Hex
US1AA-451515N	1.5	Non-Hex
US1AA-451525H	2.5	Hex
US1AA-451525N	2.5	Non-Hex
US1AA-451535H	3.5	Hex
US1AA-451535N	3.5	Non-Hex



#### Diameter Ø 5.5

Angled 15°

Code	G/H	Connection Type
US1AA-551515H	1.5	Hex
US1AA-551515N	1.5	Non-Hex
US1AA-551525H	2.5	Hex
US1AA-551525N	2.5	Non-Hex
US1AA-551535H	3.5	Hex
US1AA-551535N	3.5	Non-Hex



Diameter Ø 4.5	Code	G/H	Connection Type	Pic.
Angled 25°	US1AA-452515H	1.5	Hex	
	US1AA-452515N	1.5	Non-Hex	25°
	US1AA-452525H	2.5	Hex	G/H
	US1AA-452525N	2.5	Non-Hex	2.5
	US1AA-452535H	3.5	Hex	<b>US1AA-452525H</b> Hex
	US1AA-452535N	3.5	Non-Hex	

Diameter Ø 5.5	Code	G/H	Connection Type	Pic.
Angled 25°	US1AA-552515H	1.5	Hex	
	US1AA-552515N	1.5	Non-Hex	25°
	US1AA-552525H	2.5	Hex	
	US1AA-552525N	2.5	Non-Hex	<b>G/H</b>
	US1AA-552535H	3.5	Hex	<b>US1AA-552525H</b> Hex
	US1AA-552535N	3.5	Non-Hex	

## **Temporary Abutment**

Using a 1.28 Hex driver

Recommended torque for fastening : ≤ 30Ncm

Packaging and order: There are two pieces in the package

(abutment with screw). and for order use US1TA code with the desired size

For making provisional restoration Available in both hex and non-hex

Scale of pic is 1:1.5mm



Coding Sample: US1TA-4515H

Diameter Ø 4.5	Code	G/H	Connection Type	Pic.
	US1TA-4515H	1.5	Hex	
	US1TA-4515N	1.5	Non-Hex	<b>G/H</b> 1.5
				<b>US1TA-4515H</b> Hex

## **CCM Abutment**

(Cobalt Chromium Molybdenum)

Using a 1.28 Hex driver

Recommended torque for fastening :  $\leq$  35Ncm


Packaging and order: There are two pieces in the package

(abutment with screw). and for order use US1CA code with the desired size

Available in both hex and non-hex

Melting temperature of CCM: 1300~1400°c

Scale of pic is 1:1.5mm



Coding Sample: US1CA-4510H

Diameter Ø 4.5	Code	G/H	Connection Type	Pic.
	US1CA-4510H	1.0	Нех	<b>Diameter (Ø)</b> 4.5
	US1CA-4510N	1.0	Non-Hex	
				<b>G/H</b> 1.0
0	A Abstract			<b>US1CA-4510H</b> Hex

## **Ti-base Abutment**

## for Cerec

Packaging and order: There are 3 pieces in the package

(Ti-Base, Screw and scan body in non-sterile.). and for order use US1TB code

with the desired size

Non-sterile.

Single use only.

Mesostructure can be adhere on the Ti-Base.

The adhesive parts fixed on the implant with screw in the patient's mouth.

The scan body is only for scanning the implant position to create the design.

Ti-Base has various forms that compatible with each implant system.

Scale of pic is 1:1.5mm



Coding Sample: US1TB-4546RN-L

Code	Diameter(Ø)	н	Connection Size
US1TB-3546RN-L	3.5	4.6	RN
US1TB-4546RN-L	4.5	4.6	RN
US1TB-5746RN-L	5.7	4.6	RN



## Lab Analog

Replicates the fixture

Packaging and order: There is one piece in the package and for order use

US1LA code with the desired size

Scale of pic is 1:1.5mm



**Coding Sample: US1LA-SE** 

Diameter Ø 4.5

Н Code US1LA-SE 12



## **Impression Coping**

## Pick-up

Using a 1.28 Hex driver

Recommended torque for fastening: ≤ 5Ncm

Packaging and order: There are two pieces in the package

(impression with guide pin). and for order use US1IC code with the desired size

pick-up: Used for open tray technique

Scale of pic is 1:1.5mm



**Coding Sample :US1IC-P4015NL** 

Diameter Ø 4.0	Code	н	Connection Type	Screw Size	Pic.
Pick-up	US1IC-P4011HS	11	Hex	Short	4401
	US1IC-P4011NS	11	Non-Hex	Short	<b>H</b> 21
	US1IC-P4015HL	15	Hex	Long	
	US1IC-P4015NL	15	Non-Hex	Long	US1IC-P4015NL Non-Hex
Diameter Ø 4.5	Code	н	Connection Type	Screw Size	Pic.
Pick-up	US1IC-P4511HS	11	Hex	Short	
	US1IC-P4511NS	11	Non-Hex	Short	<b>H</b> 21
	US1IC-P4515HL	15	Hex	Long	
	US1IC-P4515NL	15	Non-Hex	Long	<b>US1IC-P4515NL</b> Non-Hex
Diameter Ø 5.5	Code	н	Connection Type	Screw Size	Pic.
Pick-up	US1IC-P5511HS	11	Hex	Short	
	US1IC-P5511NS	11	Non-Hex	Short	<b>H</b> 21
	US1IC-P5515HL	15	Hex	Long	
	US1IC-P5515NL	15	Non-Hex	Long	US1IC-P5515NL Non-Hex
Diameter Ø 6.5	Code	н	Connection Type	Screw Size	Pic.
Pick-up	US1IC-P6511HS	11	Hex	Short	
	US1IC-P6511NS	11	Non-Hex	Short	<b>H</b> 21
	US1IC-P6515HL	15	Hex	Long	7
	US1IC-P6515NL	15	Non-Hex	Long	<b>US1IC-P6515NL</b> Non-Hex

## **Impression Coping**

## Transfer

Using a 1.28 Hex driver

Recommended torque for fastening :  $\leq$  5Ncm

Packaging and order: There are two pieces in the package

(impression with guide pin). and for order use US1IC code with the desired size

transfer: Used for Closed Tray (Transfer) technique

Scale of pic is 1:1.5mm



Coding Sample: US1IC-T4015NL

Diameter Ø 4.0	Code	н	Connection Type	Screw Size	Pic.
Transfer	US1IC-T4011HS	11	Hex	Short	
	US1IC-T4011NS	11	Non-Hex	Short	<b>H</b> 15
	US1IC-T4015HL	15	Hex	Long	<b>U</b>
	US1IC-T4015NL	15	Non-Hex	Long	US1IC-T4015NL Non-Hex
Diameter Ø 4.5	Code	Н	Connection Type	Screw Size	Pic.
Transfer	US1IC-T4511HS	11	Hex	Short	<b>H</b> 15
	US1IC-T4511NS	11	Non-Hex	Short	<b>H</b> 13
	US1IC-T4515HL	15	Hex	Long	
	US1IC-T4515NL	15	Non-Hex	Long	US1IC-T4515NL Non-Hex
Diameter Ø 5.5	Code	G/H	Connection Type	Screw Size	Pic.
Transfer	US1IC-T5511HS	11	Нех	Short	<b>H</b> 15
	US1IC-T5511NS	11	Non-Hex	Short	H 15
	US1IC-T5515HL	15	Hex	Long	
	US1IC-T5515NL	15	Non-Hex	Long	<b>US1IC-T5515NL</b> Non-Hex
Diameter Ø 6.5	Code	G/H	Connection Type	Screw Size	Pic.
Transfer	US1IC-T6511HS	11	Hex	Short	<b>H</b> 15
	US1IC-T6511NS	11	Non-Hex	Short	
	US1IC-T6515HL	15	Hex	Long	
	US1IC-T6515NL	15	Non-Hex	Long	US1IC-T6515NL Non-Hex

## **Multi Straight Abutment**

Using a delivery holder

Recommended torque for fastening :  $\leq$  30Ncm

Packaging and order: There are two pieces in the package (abutment with screw).

and for order use US1MA code with the desired size

Scale of pic is 1:1.5mm



**US1MA-4810N** 

Diameter Ø 4.8	Code	G/H	Connection Type	Crown Connection	Pic.
	US1MA-4810N	1.0	Non-Hex	Hex	<del>.</del>
	US1MA-4820N	2.0	Non-Hex	Hex	<b>G/H</b> 2.5
	US1MA-4830N	3.0	Non-Hex	Hex	
	US1MA-4840N	4.0	Non-Hex	Hex	
	US1MA-4850N	5.0	Non-Hex	Hex	US1MA-4810N

## **Multi Angled Abutment**

Using a delivery holder

Recommended torque for fastening: ≤ 30Ncm

Packaging and order: There are two pieces in the package (abutment with screw).

and for order use US1MA code with the desired size

Scale of pic is 1:1.5mm

2 Kinds of angulations, 17° and 30°  $\,$ 



#### **Coding Sampling: US1MA-4825N**

Diameter Ø 4.8	Code	G/H	Connection Type	Crown Connection	Pic.
Angled 17°	US1MA-481710H	1	Hex	Non-Hex	<b>D(Ø)</b> 4.8
	US1MA-481720H	2	Hex	Non-Hex	
	US1MA-481730H	3	Hex	Non-Hex	
	US1MA-481740H	4	Hex	Non-Hex	US1MA-481710H
Diameter Ø 4.8	Code	G/H	Connection Type	Crown Connection	Pic.
Angled 30°	US1MA-483010H	1	Hex	Non-Hex	<b>D(Ø)</b> 4.8
	US1MA-483020H	2	Hex	Non-Hex	
	US1MA-483030H	3	Hex	Non-Hex	I
	US1MA-483040H	4	Hex	Non-Hex	US1MA-483010H

## **Multi Temporary Abutment**

Using a 1.28 Hex driver

Recommended torque for fastening : ≤ 30Ncm

Packaging and order: There are two pieces in the package (abutment with screw).

and for order use US1MT code with the desired size

For making provisional restoration Available in both hex and non-hex

Scale of pic is 1:1.5mm



US1MT-4815N

Diameter Ø 4.8	Code	G/H	Connection Type
	US1MT-4815H	1.5	Hex
	US1MT-4815N	1.5	Non-Hex



## **Multi CCM Abutment**

(Cobalt Chromium Molybdenum)

Using a 1.28 Hex driver

Recommended torque for fastening :  $\leq 20$ Ncm

Packaging and order: There are two pieces in the package (abutment with screw).

and for order use US1MC code with the desired size

Available in both hex and non-hex

Scale of pic is 1:1.5mm



Diameter Ø 4.8	Code	G/H	Connection Type	Pic.
	US1MC-4815H	1.5	Hex	
	US1MC-4815N	1.5	Non-Hex	
				<b>G/H</b> 1.5
				<b>US1MC-4815N</b> Non-Hex

## **Multi-unit Impression Coping**

Using a 1.28 Hex driver

Recommended torque for fastening :  $\leq$  5Ncm

Packaging and order: There are two pieces in the package (impression with guide pin).

and for order use USMI code with the desired size

Scale of pic is 1:1.5mm



Coding Sample: USMI-P4811

Pic.

Diameter Ø 4.8	Code	Туре	Н
	USMI-P4811	Pick-Up	11



## **Multi-unit LAB Analog**

Lab Analog for Multi Abutment

Packaging and order : There is one piece in the package and for order use  $% \left\{ 1,2,...,2,...\right\}$ 

USML code with the desired size

Scale of pic is 1:1.5mm



**Coding Sample: USML-48** 

Pic.


Code	Diameter(Ø)
USML-48	4.8



IISMI -4

## **Ball Abutment**

Retaining overdenture with O-ring system Recommended torque for fasting: 30Ncm Scale of pic is 1:1.5mm



**Coding Sample: US1BA-3550** 

Diameter Ø 3.5	Code	G/H	Pic.
	US1BA-3500	0	
	US1BA-3610	1.0	D (Ø)
	US1BA-3520	2.0	
	US1BA-3530	3.0	GH
	US1BA-3540	4.0	The state of the s
	US1BA-3550	5.0	US1BA-3550

## **Ball Attachment**

Packaging: There are two Pisces in the Package housing or retainer with o-ring Scale of pic is 1:1.5mm



Coding Sample: US10R-50

Diameter Ø 5.0	Code	Туре	Pic.
	US1BC-50	Housing	<b>a</b>
	US1RT-50	Retainer	
	US10R-50	O-Ring	

# SURGICAL KITS

# KITS INSTRUMENTS DRILLING SEQENCES








#### Symphony 1 Surgical kit

Bone Level Submerged Type Stopper Kit Symphony 1 implant

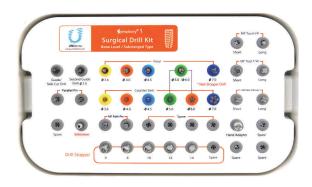

#### Symphony All Surgical Kit

Universal Drills types Stopper Kit Universal Drivers Types



#### Symphony Prosthetic Kit

Universal Drivers Types






## **Symphony 1 Surgical Kit**

Bone Level Submerged Type (Stopper Kit)



Bone Level Submerged Type Stopper Kit Used for Symphony 1 implant

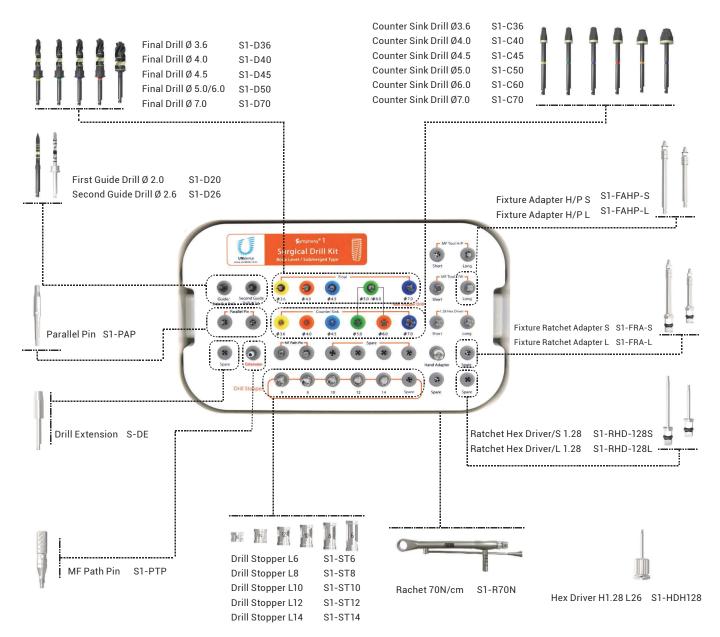



#### **Guide Drill**

Name	Code	Pic.
First Guide Drill Ø2.0	S1-D20	
Second Guide Drill Ø2.6	S1-D26	

#### Final Drill

Name	Code	Pic.
Final Drill Ø3.6	S1-D36	
Final Drill Ø4.0	S1-D40	
Final Drill Ø4.5	S1-D45	
Final Drill Ø5.0/6.0	S1-D50	
Final Drill Ø7.0	S1-D70	

#### Counter Sink

#### Path Pin

Name	Code	Pic.
MF Path Pin	S1-PTP	

Drill Stopper	Name	Code	Pic.
	Drill Stopper L6	S1-ST6	
	Drill Stopper L8	S1-ST8	
	Drill Stopper L10	S1-ST10	
	Drill Stopper L12	S1-ST12	a.
	Drill Stopper L14	S1-ST14	<u></u>
Parallel Pin	Name	Code	Pic.
	Parallel Pin	S1-PAP	
Fixture Adapter	Name	Code	Pic.
Handpiece	Fixture Adapter H/P S	S1-FAHP-S	
	Fixture Adapter H/P L	S1-FAHP-L	
Hex Driver	Code	Code	Pic.
for Ratchet	Ratchet Hex Driver/S 1.28	S1-RHD-128S	
	Ratchet Hex Driver/L 1.28	S1-RHD-128L	
Hex Driver	Code	Code	Pic.
for Hand	Hex Driver H1.28 L26	S1-HDH128	



Fixture Ratchet	Code	Code	Pic.
Adapter	Fixture Ratchet Adapter S	S1-FRA-S	
	Fixture Ratchet Adapter L	S1-FRA-L	
Drill Extension	Code	Code	Pic.
	Drill Extension	S-DE	
Depth Gauge	Code	Code	Pic.
	Depth Gauge	S1-DG	
Rachet 70N/cm	Code	Code	Pic.
	Rachet 70N/cm	S1-R70N	O THE




## **Symphony Prosthetic Kit**



#### **About Symphony Prosthetic Kit**

Al System Prosthetic Kit consists of variously sized prosthetic drivers compatible with most prosthetic hand adapters and ratchets

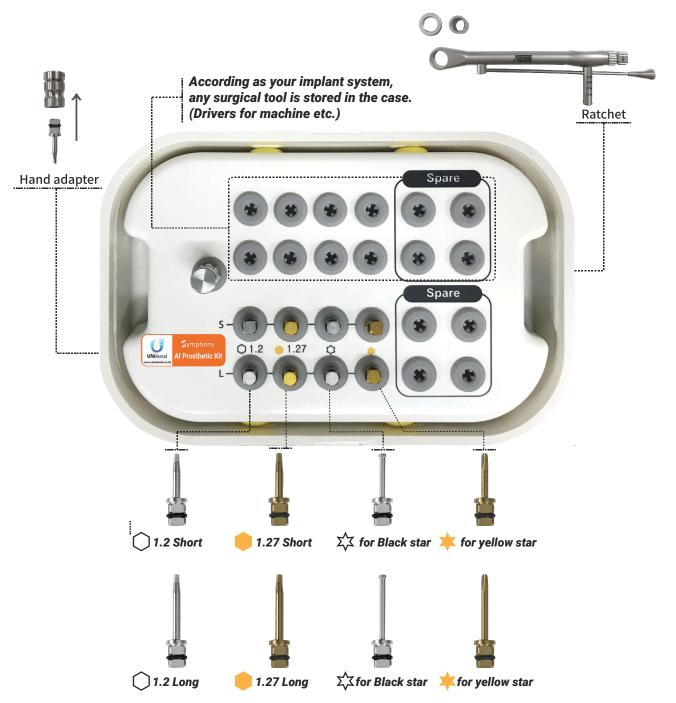



## Symphony All Surgical Kit




#### **About Symphony All Surgical Kit**

The exceptional sharpness of All Surgical Kit Drill minimizes needless bone loss and helps inserted fixture get better Fixation by penetrating into hard bone swiftly


All Surgical Kit Stopper is easy to use and guarantees accurate drilling at all times

All Surgical Kit consists of variously sized drills and drivers which cover most implant systems around the globe

The compact size of ALL Surgical Kit allows you to get easy access to various sterilization equipments

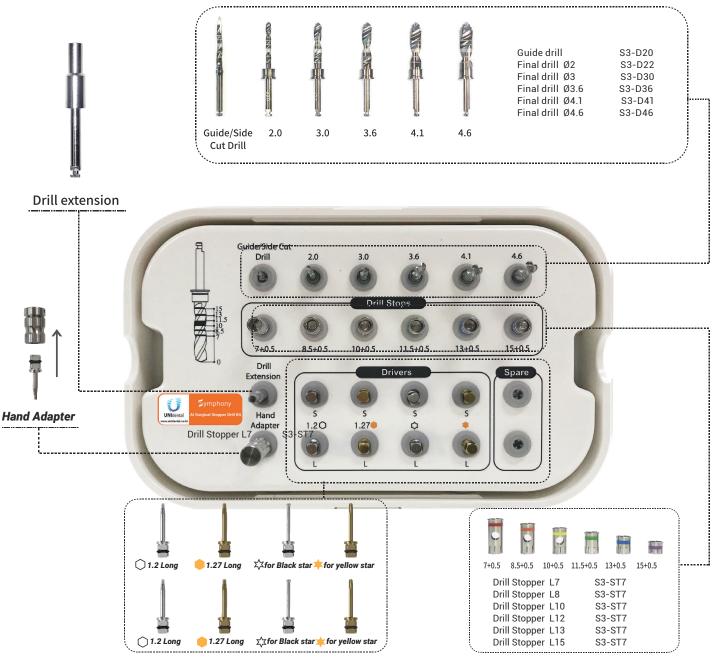


# SURGICAL Protocols

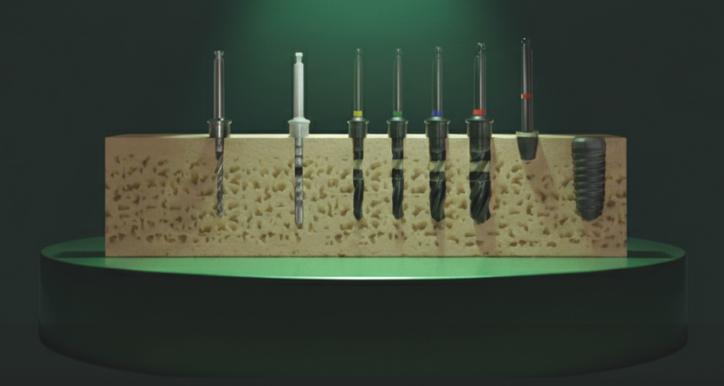







#### Diameter Ø 3.6

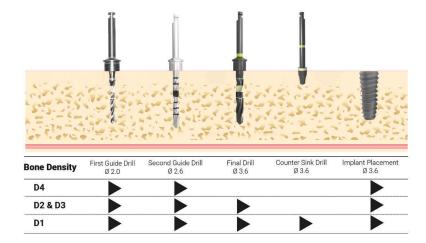

#### Diameter Ø 4.0

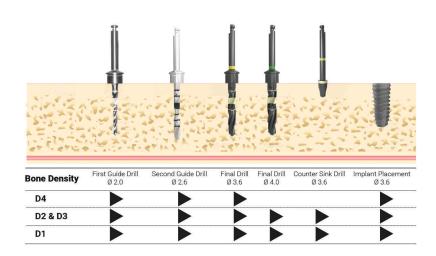


#### Diameter Ø 4.5

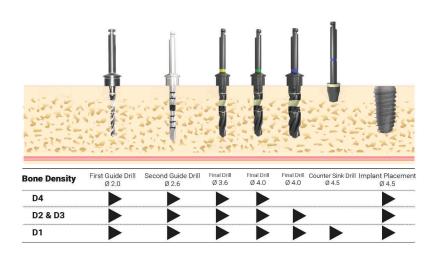





#### Diameter Ø 5.0

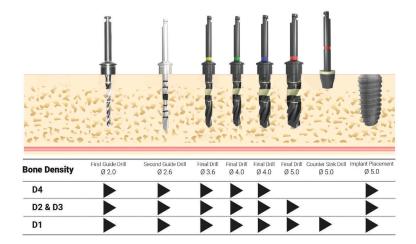

## Diameter Ø 6.0

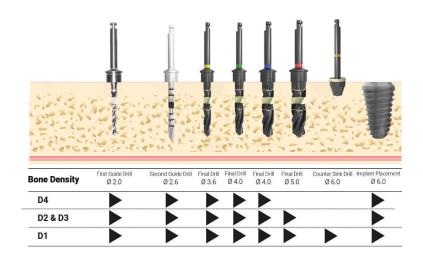

#### Diameter Ø 7.0

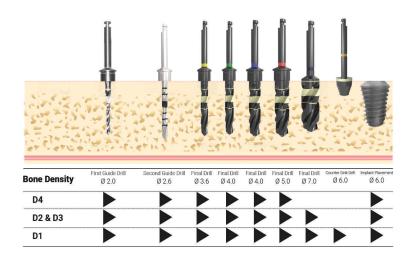

## Clinical case report

## **UNI**dental




## CASE 1

Patient Specifications: Gender: Male / Age: 42 years old /

Packaging and order: No systemic disease

**Implant treatment specifications:** Implant area: 7 lower right / Implant size: 4012









Pre implant

Implant surgery

Final prosthesis

Follow up 3yrs



## CASE 2

Patient Specifications: Gender: Female / Age: 39 years old /

Packaging and order: No systemic disease

Implant treatment specifications: Implant area: 5 and 6 lower left and 6 lower right

/ Implant size: 3 pcs. 4010









Pre implant

Implant surgery

Final prosthesis

Follow up 4yrs



## CASE 3

Patient Specifications: Gender: Male / Age: 71 years old /
Packaging and order: high blood pressure, heart disease and diabetes
Implant treatment specifications: Implant area: 1, 3 and 6 upper right,
4, 5 and 6 lower left / Implant size: 4 pcs 3610 and 2 pcs 3612









Pre implant

Implant surgery

Final prosthesis

Follow up 5yrs

Composer:	Date:
Title:	No.:
6	
<u> </u>	
<u> </u>	
1	
1	
2	
2	
<del></del>	
<u> </u>	
-0	
6	
§ .	
<u>\$</u>	
6	
<u>\$</u>	
•	
6	
6	
6	
-V	
6	







#### **Unidental Co.,Ltd**

#E Dong-4180Ho, Gmtechnopark,60, Haan-ro, Gwangmyeong-si, Gyeonggi-do, Republic of South Korea Tel:  $+82\ 2\ 898\ 8715$  Fax:  $+82\ 2\ 897\ 8715$ 

www.symphonyimplant.com